

Contents

ASSAY PROCESS.....	2
Receptor Immobilisation (Surface Preparation)	2
Ligand Binding and Dissociation (Sample Injection and Wash-off Intervals)	2
Surface Regeneration (Bound Ligand Removal)	2
RECEPTOR IMMOBILISATION	3
Direct Covalent Coupling	4
Streptavidin-Biotin Capture	4
His-tag – Nickel NTA Capture	4
Myc or FLAG-tag Capture	5
Specific Antibody Capture.....	5
Transmembrane Receptor Capture	5
LIGAND BINDING AND DISSOCIATION	5
Sample Injection	6
Sample Wash-Off	6
Surface Regeneration.....	6
DATA ANALYSIS	7
Data Output	7

ASSAY PROCESS

SPR-based kinetic affinity measurements are performed using a Biacore T200 instrument capable of automated or manual surface preparation, fully-automated injection of test samples in 96-well or 384-well formats, and output of SPR data as proprietary datafiles for evaluation with Biacore BiaEval software. The process for generation of SPR kinetic affinity data has three stages, as described below.

Receptor Immobilisation (Surface Preparation)

This stage is required to coat the biosensor surface with the target receptor (protein) to which the test compound (ligand) will bind. A variety of different immobilization / capture strategies are available, depending on the nature of the receptor.

Usually, a control receptor (protein) to which the test compound won't bind, is also coated onto a reference surface to act as a 'blank'. This allows subtraction of bulk buffer effects, such as changes due to the presence of dimethylsulphoxide (DMSO) in the sample during the sample binding phase, that is consistent across all surfaces.

Ligand Binding and Dissociation (Sample Injection and Wash-off Intervals)


After establishing a stable baseline with buffer alone flowing over the sensor surface, sample is passed over the receptor surface for binding to occur. This period defines the binding association rate. After a defined interval, sample flow ceases and flow of buffer alone is resumed. This allows the bound ligand to wash off, defining the dissociation rate. The duration of the ligand binding and ligand dissociation intervals needs to be sufficient to measure binding kinetics but should be as short as practical to conserve reagents and increase sequential sample throughput.

Surface Regeneration (Bound Ligand Removal)

Samples are passed over the sensor surface sequentially. For low-affinity ligands, dissociation can be complete (back to initial baseline level) within a few minutes, allowing the next sample to be injected onto a 'clean' sensor surface after a short delay. For high affinity ligands, complete dissociation back to baseline can take hours, but only a few minutes of dissociation rate data are required for analysis. To remove all bound ligand from the sensor surface before the next sample is injected, a 'regeneration' step can be used. This process applies a mild pH change, ionic strength change, or some other biophysical process to rapidly dissociate the

ligand from the receptor surface without damaging or denaturing the receptor protein. After returning to baseline with standard buffer flow, the next sample can be injected.

Example Sample Association, Dissociation and Regeneration Cycle

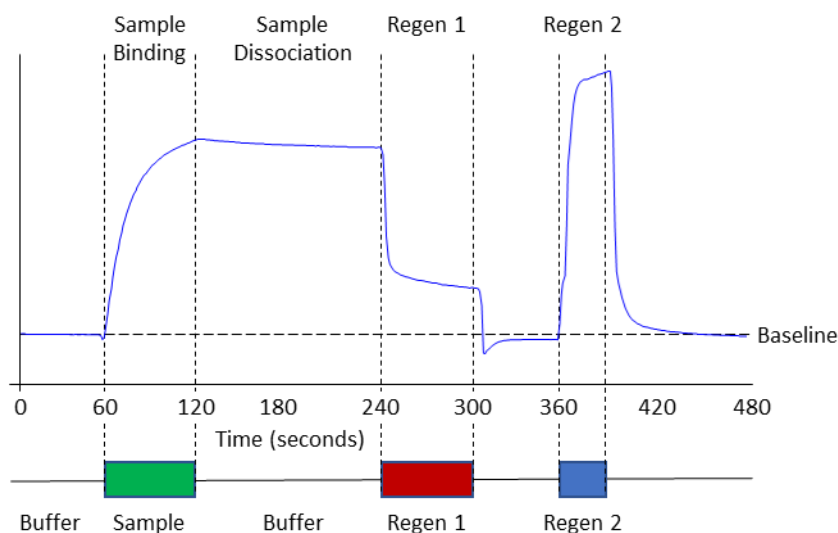

It is important to optimize the regeneration conditions at the start of the sample testing process. This ensures that the 'clean' baseline level is achieved before each new sample is tested, avoiding accumulation of traces of previous compounds on the surface. It also ensures that cumulative denaturing of the receptor surface over consecutive binding, dissociation and regeneration cycles is avoided. Together, these ensure that the binding capacity of the surface remains unchanged throughout the assay, allowing meaningful sample to sample comparison.

RECEPTOR IMMOBILISATION

The immobilization method used to couple the receptor onto the biosensor surface is dependent on the nature of the target receptor and any modification that may have been made to it to facilitate the coupling process. Examples of possible immobilization strategies and the recommended biosensors are given below.

The amount of receptor coupled / captured onto the biosensor surface determines the amplitude of the sample binding response as a ratio of the molecular masses of the receptor and ligand, i.e.:

MWt of receptor = 50,000 Da; 100 RU captured onto biosensor

MWt of ligand = 500 Da; expected binding response = $(500/50,000) \times 100 = 1$ RU

Therefore, 100 RU of receptor capture would be the minimum sufficient to detect a binding response in this case (at a detection threshold of ~0.2 RU). Capturing too little receptor onto the biosensor means that a ligand binding response cannot be detected. However, capturing too much receptor can have detrimental effects, such as steric hindrance or ligand depletion at the sensor surface. We usually adjust the receptor capture level to give an expected ligand binding response of up to 10 RUs.

Direct Covalent Coupling




A purified receptor protein can be covalently-coupled onto carboxymethyl dextran (CM3, CM4, CM5 or CM7) biosensor surfaces. A range of dextran chain lengths and carboxyl group densities are provided to optimize receptor coupling. Side-chain amine coupling using EDC-NHS chemistry is typical, though thiol and other coupling chemistries are also available. This method produces a stable biosensor surface that can be used for many ligand binding and regeneration cycles. Purified receptor is required to avoid coupling other proteins that may be present in an unpurified mixture onto the surface. The protein must be supplied in a buffer that does not contain Tris/TRIZMA (tris(hydroxymethyl)aminomethane) because this neutralizes the amine-coupling chemistry. This is one of our preferred coupling protocols.

Streptavidin-Biotin Capture



Biotinylated receptor can be captured onto a precoated streptavidin (SA) biosensor surface. Purified receptor can be directly biotinylated using commercially available kits before injection onto the surface. This method also produces a stable biosensor surface that can be used for many ligand binding and regeneration cycles. It is our preferred capture protocol.

His-tag – Nickel NTA Capture



Recombinant receptor protein incorporating a 4 x his tag can be captured onto a pretreated nickel- nitrilotriacetic acid (NTA) biosensor surface. The receptor does not need to be purified – only the his-tagged protein will be captured onto the surface.

Myc or FLAG-tag Capture



Recombinant receptor protein incorporating a Myc-tag or FLAG-tag can be captured onto an anti-Myc or anti-Flag antibody surface covalently-coupled onto a carboxymethyl dextran (CM5 sensor). Alternatively, the anti-Myc or anti-Flag antibody can be captured onto pretreated (Protein A, G or L) biosensors surfaces. The receptor does not need to be purified – only the myc-tagged or FLAG-tagged protein will be captured onto the surface. However, this approach can be affected by the very slow dissociation of the receptor from the capture antibody, reducing the binding capacity of the surface over repeated binding cycles. Surface regeneration may also remove the tagged receptor from the capture antibody. These issues can be overcome by re-capturing the tagged receptor onto the antibody surface after each binding and regeneration cycle but will require larger quantities of receptor to do this.

Specific Antibody Capture



Native receptor without a tag can be captured onto a specific antibody, either covalently-coupled onto a carboxymethyl dextran surface (CM5 sensor), or captured onto pretreated (Protein A, G or L) biosensor surfaces. The receptor does not need to be purified – only the native receptor recognized by the specific antibody will be captured onto the surface. As for Myc-tag and FLAG-tag antibody capture, this approach can be affected by the dissociation of the receptor from the specific capture antibody and/or surface regeneration.

Transmembrane Receptor Capture



Purified transmembrane protein can be reconstituted into synthetic bilayer lipid membrane micelles and then captured onto a lipophilic (L1) biosensor surface. Use of recombinant receptors in native membrane micelles (prepared from cultured cell membranes), is not recommended because receptor expression, even if highly-expressed, can still be insufficient to detect a drug binding signal. Additionally, the membrane micelles contain a heterogeneity of unknown proteins which may also bind the test compound.

LIGAND BINDING AND DISSOCIATION

Samples can be prepared for analysis in either 96-well or 384-well formats. Usually 5 concentrations of the sample compound, e.g. 1 nM, 3 nM, 10 nM, 30 nM and 100 nM, are

tested sequentially, in duplicate. Samples are usually tested against the specific target receptor and a control, reference surface. However, up to three different target receptors and a control surface may be used (i.e. up to four sample analysis channels are available). Automated sample injection can proceed for up to 48 hours, depending on the number of samples and dilutions required, and the durations of each injection, as described below. It is imperative that the target receptor and test compounds remain stable in aqueous solution over this period.

Sample Injection

The buffer flow rate used for sample injection is typically 10 $\mu\text{l}/\text{minute}$. For small molecule ligands with fast association rates, an injection duration of 60 seconds is usually sufficient to achieve a full binding response. For ligands with slower association rates, a binding duration of up to 5 minutes may be required. Consequently 10 to 50 μl + 30 μl handling excess is required of each sample dilution, dependent on the injection duration.

Sample Wash-Off

Immediately after sample injection is complete, buffer flow is resumed to allow the ligand to dissociate. As above, for small molecule ligands with fast dissociation rates, a wash-off duration of 60 seconds is usually sufficient to achieve full dissociation. For ligands with slower dissociation rates, a wash-off duration of up to 10 minutes may be required to be able to measure appreciable dissociation. This affects the duration of each sample injection and dissociation cycle.

Surface Regeneration

For small molecule, low affinity ligands with fast dissociation rates, regeneration cycles may not be required to return the biosensor to a stable baseline before injection of the next sample. However, for higher affinity, more slowly dissociating ligands (as shown in the example above), we usually regenerate the surface with one or two short injections of mild acid or alkali, high or low salt, or other chemical treatments to rapidly dissociate any remaining bound ligand from the receptor. We usually perform a preliminary study to identify and optimize appropriate regeneration conditions before commencing sample testing. The regeneration conditions are validated by repeating several binding and regeneration cycles using a standard reference compound to show the consistency of binding response amplitude and return to baseline for each cycle. Using additional regeneration steps in each sample binding cycle has further impact on cycle duration.

DATA ANALYSIS

Automated data analysis is performed using proprietary Biacore SPR evaluation software. The continuous sequence of cycles of sample association and dissociation data for each flow channel is automatically cut into segments corresponding to each experimental cycle and then overlaid. Data for each channel are aligned to the start of the sample injection period for each injection cycle, then set to a zero baseline value. Reference channel (control surface) responses are then subtracted from the test channel (target receptor surface) response(s) to remove bulk sample effects (e.g. to correct for DMSO present in the sample). Alternatively, or in addition, a blank cycle response (e.g. buffer + DMSO but no test compound) can be subtracted from each flow channel response separately to control for buffer differences.

After selecting the appropriate association and dissociation regions of the binding responses (avoiding artifacts at the start and end of each injection), data are globally fitted to a four-parameter non-linear curve fit model using the 'least squares' fit method.

Data Output

Data output for each test compound comprises a kinetic affinity chart showing the aligned binding response data for all concentrations tested, and the 'global best fit' line for each concentration plotted through the response data. This provides a visual indication of the quality of the binding response. Kinetic affinity data calculated from the best fit curves are also tabulated for each test compound. These comprise: association rate (k_a); dissociation rate (k_d); affinity dissociation constant (K_D), and goodness of fit (R^2).